



Bante210 Benchtop pH Meter

Instruction Manual

Introduction


Thank you for selecting the Bante210 benchtop pH meter. This manual provides a step-by-step guide to help you operate the meter, please carefully read the following instructions before use.

Unpacking


Before unpacking, ensure that the current work environment meets following conditions.

- Relative humidity is less than 80%.
- Ambient temperature is greater than 0°C and less than 60°C.
- No potential electromagnetic interference.


The following list describes the standard components of the meter. After the unpacking, please check all components are complete. If any are damaged or missing, please contact nearest distributor.

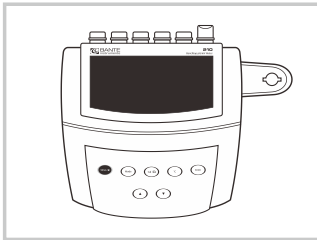


Bante210 pH Meter

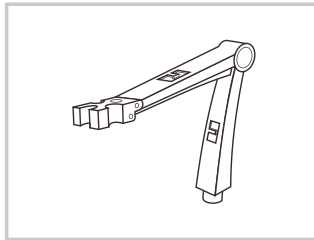


Electrode Arm

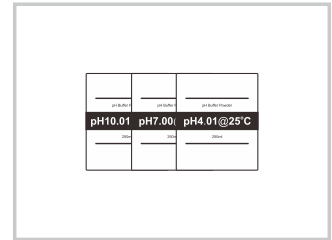


pH4.01/7.00/10.01 Buffer Pouches

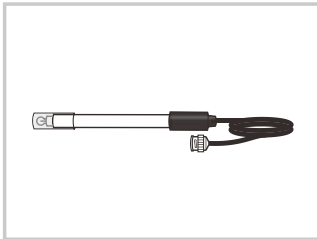

pH Electrode

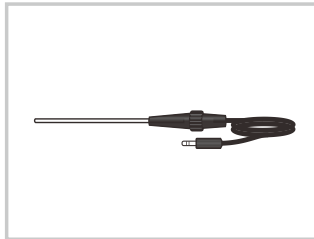


TP-10K Temperature Probe

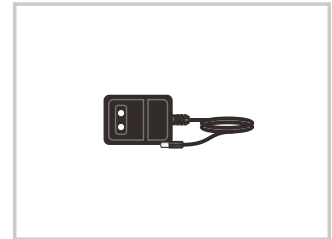






DC9V Power Adapter

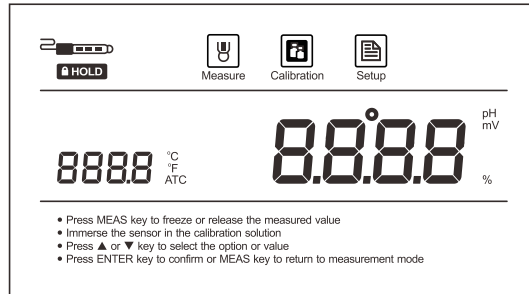Display

The meter is equipped with an easy-read LCD display that used to show measured values and mode icons. The following table describes the function of each icon.





INDEX:

 Measurement	Measurement mode icon: Indicates the meter is in the measurement mode.		Electrode slope icon: Indicates the average slope of the pH electrode.
 Calibration	Calibration mode icon: Indicates the meter is in the calibration mode.		Hold icon: Indicates the measuring value has been locked.
 Setup	Setup mode icon: Indicates the meter is in the setting mode.	ATC	Automatic Temperature Compensation: Indicates the temperature compensation is enabled.


Keypad

The meter has a succinct membrane keypad, names and symbols describe the each function key controls.

KEY	FUNCTION
MEAS 	<ul style="list-style-type: none"> Switches the meter ON/OFF. Locks the measured value, press the key again to resume measuring. Exits the calibration or setting and returns to measurement.
MODE	<ul style="list-style-type: none"> Toggles between pH and mV measurement modes.
CAL 	<ul style="list-style-type: none"> Starts calibration. Enters the setup menu (Press and hold the key for 3 seconds).
°C	<ul style="list-style-type: none"> Sets the temperature.
▲	<ul style="list-style-type: none"> Increase the setting value.
▼	<ul style="list-style-type: none"> Decrease the setting value.
ENTER	<ul style="list-style-type: none"> Confirms the calibration, settings or displayed options.

Connectors


The meter provides 4 connectors for connecting the various types of sensors. Listed in the below table are the details of these connectors.

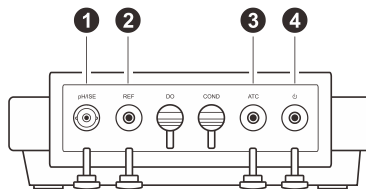

NO.	CONNECTOR	DESCRIPTION
1	pH/ISE	Used for connecting the pH or ORP electrode.
2	REF	Used for connecting the reference electrode.
3	ATC	Used for connecting the temperature probe.
4	⏻	Used for connecting the power adapter.

Installing the Electrode Holder


Take out the electrode arm from the packaging. The base plate of the electrode holder has an irregular round hole, the electrode arm has a connecting rod. Insert the connecting rod into the irregular round hole and swivel the electrode arm 90°. Electrode holder is now ready to swing into desired position.

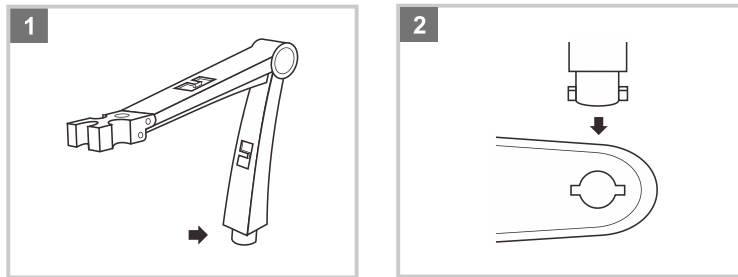

Adjustment of Electrode Arm


After installation, if the electrode arm automatically rises or falls, you need to adjust the screws until arm locate at any position.

1. Remove the plastic cover from the electrode arm.
2. Use the screwdriver to tighten the screw moderately.
3. Insert the plastic cover to previous position. Installation is completed.

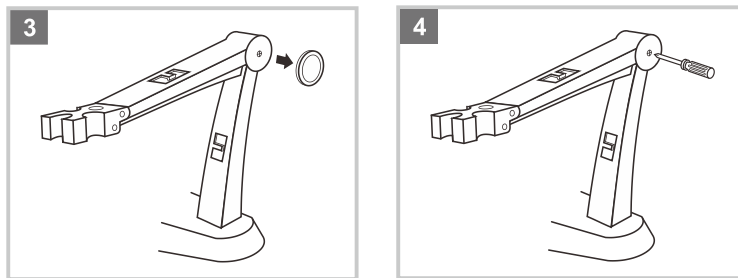


Connecting the Electrode

1. Take out the pH electrode from the packaging. Follow the steps below to place the electrode into left or right side of the electrode arm.

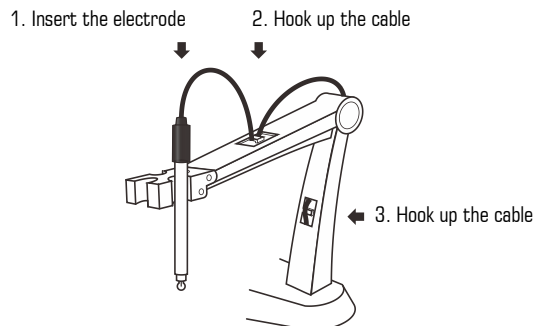


2. Insert the BNC connector into the connector socket labeled "pH/ISE". Rotate and push the connector clockwise until it locks. After the connection is completed, DO NOT pull on the cable. Always make sure that the connector is clean and dry.

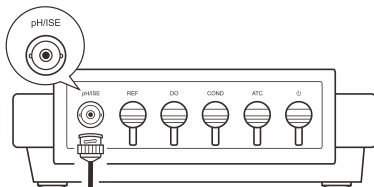


Connecting the Temperature Probe

1. Place the temperature probe into the round hole of the electrode arm.

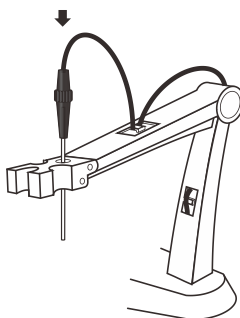


2. Insert the phone plug to the connector socket labeled "ATC". Ensure the connector is fully seated.

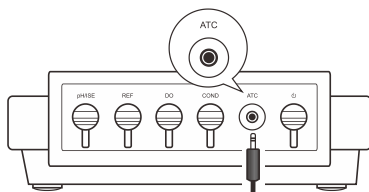

Connecting the Power Adapter

1. Before plugging in the power adapter, ensure that its voltage matches the local main voltage.
2. Insert the connector to the power socket. The meter is now ready for use.

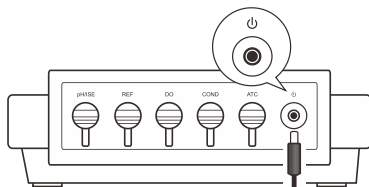

Preparing the pH Buffer Solutions

Bante210 benchtop pH meter is packaged with three pH buffer packets required for calibration.

- Open the pH7.00 buffer packet, place the powder into a 250ml volumetric flask. Pour distilled water 250ml to scale line, mix the solution until the reagent is completely dissolved.
- Preparation of pH4.01 and 10.01 standard buffer solutions are the same as above.
- Prepared standard buffer solutions should be stored in hermetically sealed glass containers.


pH Buffer 1	pH Buffer 2	pH Buffer Powder
pH10.01	pH7.00	pH4.01@25°C
250ml	250ml	250ml

Prior to Use

Remove the protective cap from the bottom of the electrode.

pH Electrode

If the glass sensitive membrane has dried out, soak the electrode in 3M KCL solution (pH adjusted to 4.0) for at least 15 minutes. DO NOT store the electrode in distilled or deionised water that will render the electrodes useless.

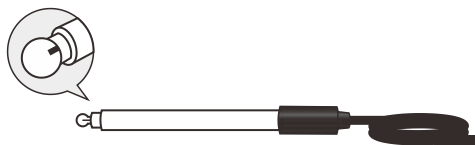

ORP Electrode (Purchase separately)

If the sensing element has dried out, soak the electrode in 4M KCL solution for at least 15 minutes.



Power On/Off

- Press the **Meas** key to turn on the meter, the display shows the measured value.
- Press and hold the **Meas** key for 5 seconds, the meter will turn off.




i To enable the Auto-Power Off feature, please refer to chapter "Setup Menu".

Setup Menu


Bante210 benchtop pH meter contains an integrated setup menu that is used to customize the displayed option to meet measurement requirements.

MENU	DESCRIPTION	OPTIONS		DEFAULT
BUF	Set the pH buffer group for calibration and auto-recognition.	USA	USA (pH4.01/7.00/10.01)	USA
		NIST	NIST (pH4.01/6.86/9.18)	
CAL	Set the number of calibration points.	1	1 point	2 points
		2	2 points	
		3	3 points	
UNIT	Set the default temperature unit.	°C	Degrees Celsius	°C
		°F	Degrees Fahrenheit	
HOLD	When the option is enabled, the meter will automatically sense a stable reading and lock the measurements.	YES	Enable	Disable
		NO	Disable	
OFF	When the option is enabled, the meter will automatically turn off if no key is pressed within 3 hours.	YES	Enable	Disable
		NO	Disable	
RST	Reset the meter to factory default settings.	YES	Enable	Disable
		NO	Disable	

Setting the Default Option

- In the measurement mode, press and hold the  key for 3 seconds to enter the setup menu.
- Press the  or  key select the desired option.
- Press the **Enter** key to confirm and move to the next menu item.
- Repeat the steps above until the meter returns to the measurement mode. Setting is completed.

- During the setting process, press the **Meas** key, the meter will exit the setup menu and return to the measurement mode.
- The Reset function will restore the meter back to factory default settings, If enabled, all of the calibration data and selected parameters will be lost or reset, the meter must be recalibrated.

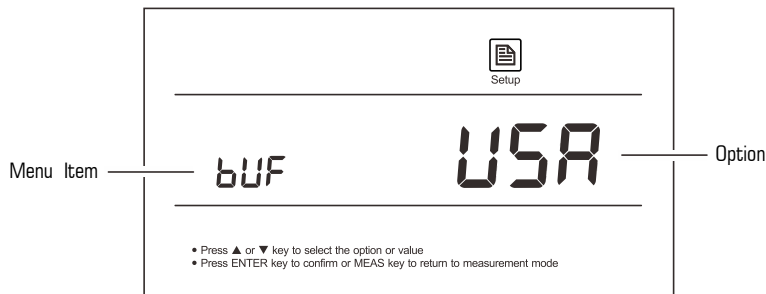


Temperature Compensation

For better accuracy, we recommend the use of either a sensor with a built-in or a separate temperature probe for the calibration or measurement.

Automatic Temperature Compensation (ATC)


Connect the temperature probe to the meter (Refer to page 5 "Connecting the Temperature Probe"). The ATC icon immediately appears on the display, the meter is now switched to the automatic temperature compensation mode.

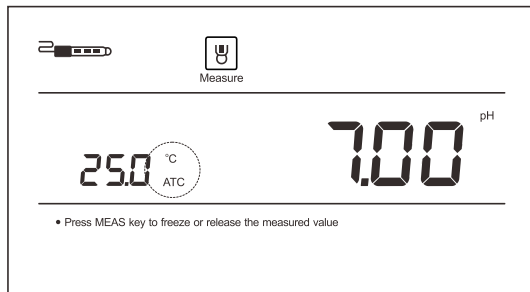

Manual Temperature Compensation (MTC)

If the meter does not detect a temperature probe, the °C icon will show on the display indicating that the meter is switched to the manual temperature compensation mode. To set the temperature value of sample, follow the steps below.

1. Press the °C key to enter the temperature setting mode.
2. Press the ▲ or ▼ key to modify the temperature value.
3. Press the **Enter** key to confirm, the meter returns to the measurement mode. Setting is completed.

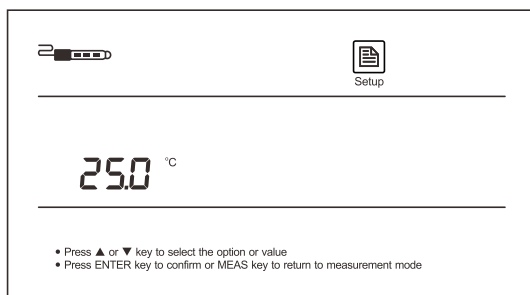

- ① During the setting process, press the ▲ or ▼ key once, the setting value will increase or decrease by 0.1. Press and hold the ▲ or ▼ key, the setting value will increase or decrease by 1.

pH Calibration

Bante210 benchtop pH meter allows 1 to 3 points calibration. We recommend that you perform at least 2 points calibration for high accuracy measurement. The meter will automatically recognize and calibrate to following standard buffer values.


USA Standard Buffers	pH4.01, 7.00, 10.01
NIST Standard Buffers	pH4.01, 6.86, 9.18

Single point calibration should only be carried out with pH7.00 or 6.86, otherwise calibration will not be accepted.



The meter must be calibrated prior to first use or new electrode replaced. To ensure accuracy, regular calibration is recommended. DO NOT reuse the pH buffer solution after calibration, contaminants in solution will affect the calibration and eventually the accuracy of the measurement.

Single Point Calibration

- 1.1 Make sure that you have selected 1 point calibration in the setup menu.
- 1.2 Rinse the pH electrode with distilled water. Press the **Cal** key, the meter shows "CAL1/pH7.00" (or "CAL1/pH6.86").

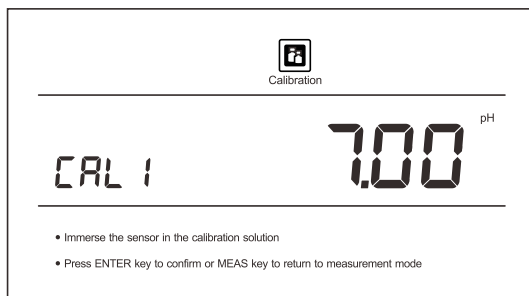


- 1.3 Place the pH electrode into the pH7.00 (or pH6.86) standard buffer solution. Stir the electrode gently to create a homogeneous solution.
- 1.4 Press the **Enter** key, the meter begins the calibration, the "Calibration" icon will continuously flashing. Wait for the reading to stabilize, the meter automatically shows "END". Single point calibration is completed.

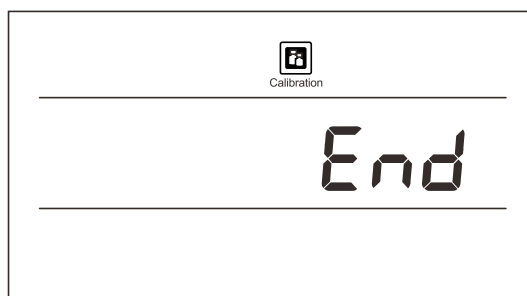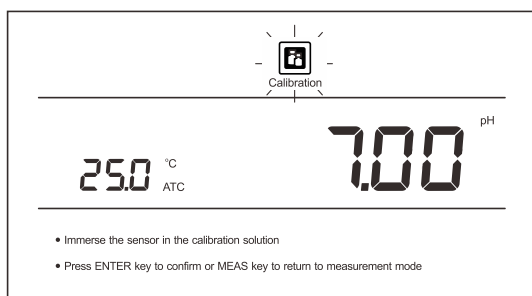


2 Points Calibration



- 2.1 Make sure that you have selected 2 points calibration in the setup menu.
- 2.2 Repeat steps 1.2 to 1.4 above. When the first calibration point is completed, the display will show "CAL2". The meter prompts you to continue with second point calibration.

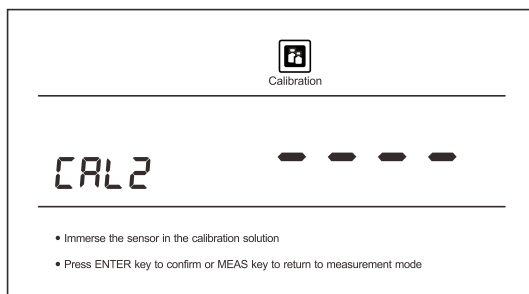

- 2.3 Rinse the pH electrode with distilled water. Place the electrode into the pH4.01 or 10.01 (pH4.01 or 9.18) standard buffer solution. Stir the electrode gently.
- 2.4 Press the **Enter** key, the meter automatically recognizes the pH buffer solution and begins the calibration (e.g., pH4.01), the "Calibration" icon will continuously flashing.

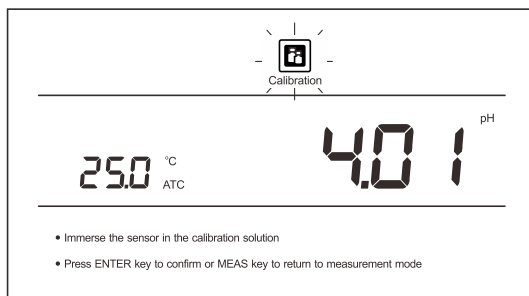


Wait for the reading to stabilize, the meter shows the electrode slope and "END". Second point calibration is completed.

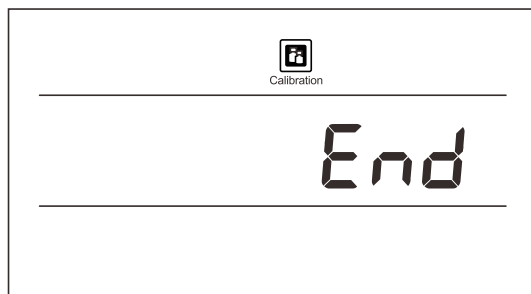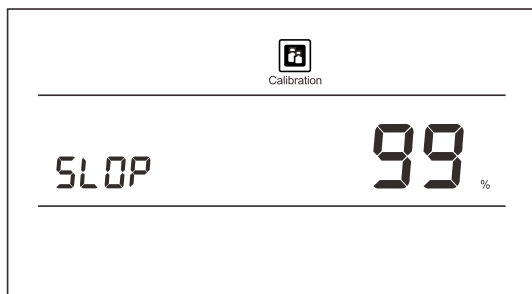


3 Points Calibration

- 3.1 Make sure that you have selected 3 points calibration in the setup menu.
- 3.2 Repeat steps 1.2 to 1.4 above. When the first calibration point is completed, the display will show "CAL2/pH4.01". The meter prompts you to continue with second point calibration.

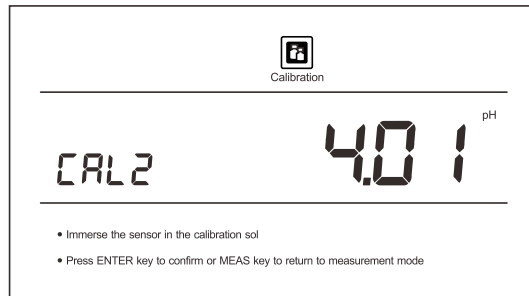

- 3.3 Rinse the pH electrode with distilled water. Place the electrode into the pH4.01 standard buffer solution. Stir the electrode gently.
- 3.4 Press the **Enter** key, the meter begins the calibration. Wait for the reading to stabilize, the display automatically shows electrode slope and "CAL3/pH10.01" (or "CAL3/pH9.18").

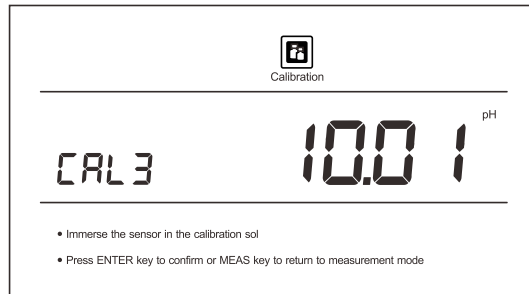

- 3.5 Rinse the pH electrode with distilled water. Place the electrode into the pH10.01 (or pH9.18) standard buffer solution. Stir the electrode gently.
- 3.6 Press the **Enter** key. Wait for the reading to stabilize, the display will show the electrode slope and "END". The meter automatically returns to the measurement mode. Calibration is completed.




- During the calibration process, if the meter shows "Err", please check the pH electrode and ensure the pH buffer solutions are fresh and uncontaminated.
- Press the **Meas** key, the meter will cancel the calibration and return to the measurement mode.
- The electrode icon (☐) shows the average slope of the pH electrode when the calibration is completed. If the slope or calibration result does not meet measurement requirements, the icon will disappear on the display.

Temperature Calibration

During the measurement process, if the temperature reading displayed differs from that of an accurate thermometer, the meter needs to be calibrated.

1. Connect the temperature probe to the meter and place into a solution with a known accurate temperature.
2. Press the **°C** key to enter the temperature setting mode.
3. Press the **▲** or **▼** key to set the temperature value.
4. Press the **Enter** key, the meter returns to the measurement mode. Calibrating is completed.

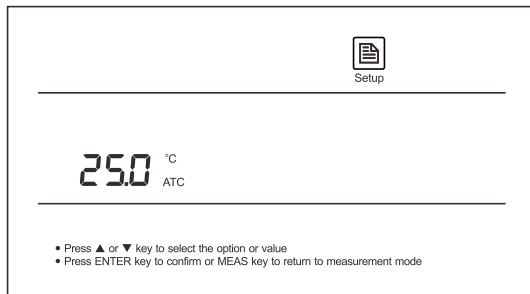


pH Measurement


- 1.1 Press the **Mode** key until the display shows the measurement unit "pH".
- 1.2 Rinse the pH electrode with distilled water to remove any impurities adhering to the probe body.
- 1.3 Place the electrode into the sample solution, stir the electrode gently.
- 1.4 Record the measured value when the reading is stable.

mV Measurement

- 2.1 Press the **Mode** key until the display shows the measurement unit "mV".
- 2.2 Rinse the electrode thoroughly with distilled water.
- 2.3 Place the electrode into the sample solution, stir the electrode gently.
- 2.4 Record the measured value when the reading is stable.

Auto-Hold

Bante210 benchtop pH meter contains an Auto-Hold feature. If enabled, the meter will automatically sense a stable reading and lock the measurements. The "HOLD" icon appears on the display. If disabled, press the  key, the meter will immediately lock the displayed value. Press the **Meas** key to resume measuring.

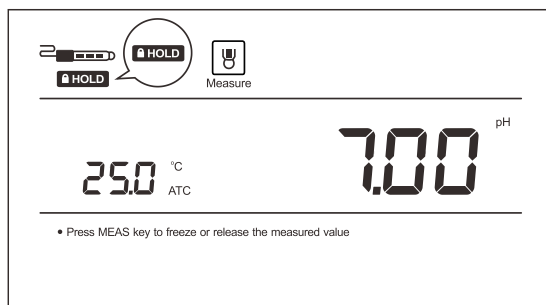

pH Electrode Care and Maintenance

Since pH electrode is susceptible to dirt and contamination, clean as necessary depending on the extent and condition of use.

- After measuring: rinse the electrode in distilled water, store the electrode into the 3M KCL solution.
- Salt deposits: soak the electrode in warm tap water to dissolve deposits, then thoroughly rinse with distilled water.
- Oil or Grease film: wash the glass sensitive membrane of electrode gently in some detergents and water. If necessary, using the alcohol to clean the sensitive membrane, then rinse with distilled water. Place the electrode in the 3M KCL solution for at least 30 minutes.
- Clogged reference junction: heat a diluted KCl solution to 60°C to 80°C. Place the electrode into the heated solution for about 10 minutes. Allow the electrode to cool in some unheated KCl solution.
- Protein deposits: prepare a 1% pepsin solution in 0.1M of HCL. Place the electrode in the solution for 10 minutes. Rinse the electrode with distilled water.

Rectivating the Electrode

If stored and cleaned properly, the electrode should be ready for immediate use. However, a dehydrated sensitive membrane may cause sluggish response. To rehydrate the sensitive membrane, immerse the electrode in a pH4.01 buffer solution for 10 to 30 minutes. If this fails, the electrode requires activation.

1. Soak the electrode in 0.1M HCl for 5 minutes.
2. Remove and rinse with deionized water, then place in 0.1M NaOH for 5 minutes.
3. Remove and rinse again, and soak in 3M KCL solution for at least 30 minutes.

Optional pH Electrodes

Bante210 benchtop pH meter comes with a general purpose pH electrode that is used to measure the pH of the liquids. If this electrode can not meet your measurement requirements, please refer to the table below to select an applicable probe.

SAMPLE TYPE	P11	P12	P13	P15	P16	P18	P19	P21	E201	E202
Agar										•
Beer	•	•	•					•	•	•
Blood Products	•	•	•					•		•
Bread, Dough						•	•			
Cement	•									
Cosmetics	•	•	•					•	•	•
Dairy Products	•	•	•				•			•
Education	•								•	•
Fats/Cream							•			
Field Use						•			•	•
Fish Products							•			•
Lab Flasks		•								
Low Ionic	•			•				•		
Meat, Cheese							•			•
Micro Samples			•							
Paint		•	•							•
Photographic										
Soil						•	•			
Surface										•
Test Tubes		•			•					
Tris Buffer					•					
Viscose Samples										•

Troubleshooting

LCD DISPLAY	CAUSE	CORRECTIVE ACTION
---	Electrode dried out	Soak the pH electrode in 3M KCL solution at least 20 minutes.
	Measured value is out of range	Check the electrode whether clogged, dirty or broken.
Err	Incorrect pH buffer solutions	Using the fresh pH buffer solutions for calibration.
	Electrode has expired	Replace the pH electrode.

Specifications

pH	Model	Bante210
	Range	-1.00~15.00pH
	Accuracy	±0.01pH
	Calibration Points	1 to 3 points
	Calibration Solutions	USA (pH4.01/7.00/10.01) or NIST (pH4.01/6.86/9.18)
	Temperature Compensation	0~100°C, 32~212°F, Manual or Automatic
mV	Range	-1999~1999mV
	Accuracy	±1mV
	Resolution	1mV
Temperature	Range	0~105°C, 32~221°F
	Accuracy	±1°C
	Resolution	0.1°C
	Calibration Points	1 point
Other	Connector	BNC
	Display	LCD (135×75mm)
	Power Requirements	DC9V, using AC adapters, 220VAC/50Hz
	Dimensions	210(L)×205(W)×75(H)mm
	Weight	1.5kg

Hazardous Substance Statement

Bante Instruments is committed to the reduction and eventual elimination of all hazardous substances in both the manufacturing process and finished products we supply. We have an active manufacturing and procurement program to minimize and eliminate the use of harmful heavy metals such as cadmium, lead, mercury and the like. New technologies and design parameters are also promoting these efforts and we expect to have little or no such materials in our product in the coming years. We welcome our customer suggestions on how to speed up these efforts.



Warranty

The warranty period for meter is one year from the date of shipment. Above warranty does not cover sensor and calibration solutions. Out of warranty products will be repaired on a charged basis. The warranty on your meter shall not apply to defects resulting from:

- Improper or inadequate maintenance by customer.
- Unauthorized modification or misuse.
- Operation outside of the environment specifications of the products.

For more information, please contact the nearest authorized distributor.



BANTE INSTRUMENTS CO., LTD
E-mail: banteinstruments@yahoo.com
Phone: +8621-6404-1598
Website: www.bante-china.com